

WUHAN HUAMEI BIOTECH CO., LTD.

Postal Address: Wuhan Hi-tech Medical Devices Park, Building B11, #818 Gaoxin Road, Donghu Hi-Tech Development Area, Wuhan, Hubei Province 430206, P.R. China

Website: www.cusabio.com www.cusabio.cn

Email: cusabio@cusabio.com Tel: +86-27-87582341

Fax: +86-27-87582341



PRECISION

Intra-assay Precision (Precision within an assay): CV%<8%

Three samples of known concentration were tested twenty times on one plate to assess.


Inter-assay Precision (Precision between assays): CV%<10%

Three samples of known concentration were tested in twenty assays to assess.

	Intra-Assay Precision			Inter-Assay Precision		
Sample	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean(µg/ml)	7.035	6.864	6.588	6.724	6.669	6.697
SD	0.020	0.021	0.020	0.034	0.035	0.036
CV(%)	3.324	3.516	3.276	5.72	5.818	6.037

TYPICAL DATA

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

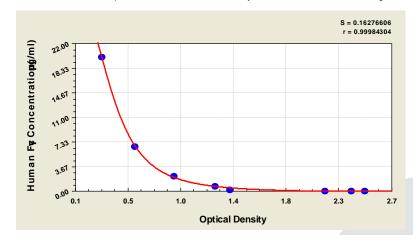

μg/ml	OD1	OD2	Average
20	0.315	0.337	0.326
6.667	0.597	0.601	0.599
2.222	0.921	0.905	0.913
0.741	1.246	1.25	1.248
0.247	1.402	1.336	1.369
0.082	2.138	2.14	2.139
0.027	2.364	2.346	2.355
0	2.483	2.451	2.467

LOD

 $0.024 \mu g/ml$

LINEARITY

To assess the linearity of the assay, samples were spiked with high concentrations of human Fcγ in various matrices and diluted with the Sample Diluent to produce samples with values within the dynamic range of the assay.

	Sample	Serum(n=4)	
1:500	Average %	95	
1.500	Range %	87-104	
1:1000	Average %	96	
1.1000	Range %	91-110	
1:2000	Average %	93	
1.2000	Range %	85-99	
1:4000	Average %	93	
1.4000	Range %	88-100	